



HAMILTON, BROOK, SMITH & REYNOLDS, P.C.

UTILITY PATENT APPLICATION TRANSMITTAL

(Only for new nonprovisional applications under 37 CFR 1.53(b))

Attorney Docket No. CYL98-01

First Named Inventor or Application Identifier

Steven A. Bogen

Express Mail Label No. EM 4824 727 56 US

APPLICATION ELEMENTS

See MPEP chapter 600 concerning utility patent application contents.

ADDRESS TO: Assistant Commissioner for Patents
Box Patent Application
Washington, DC 20231

1. ☐ Fee Transmittal Form
(Submit an original, and a duplicate for fee processing)
2. ☒ Specification [Total Pages 33]
(preferred arrangement set forth below)
 - Descriptive title of the Invention
 - Cross References to Related Applications
 - Statement Regarding Fed sponsored R & D
 - Reference to Microfiche Appendix
 - Background of the Invention
 - Brief Summary of the Invention
 - Brief Description of the Drawings (if filed)
 - Detailed Description
 - Claim(s)
 - Abstract of the Disclosure
3. ☒ Drawing(s) (35 USC 113) [Total Sheets 17]
4. Oath or Declaration / POA [Total Pages]
 - a. ☐ Newly executed (original or copy)
 - b. ☐ Copy from a prior application (37 CFR 1.63(d))
(for continuation/divisional with Box 17 completed)
[Note Box 5 below]
 - i. ☐ DELETION OF INVENTOR(S)
Signed statement attached deleting inventor(s) named in the prior application, see 37 CFR 1.63(d)(2) and 1.33(b).
5. ☐ Incorporation By Reference (useable if Box 4b is checked)
The entire disclosure of the prior application, from which a copy of the oath or declaration is supplied under Box 4b, is considered as being part of the disclosure of the accompanying application and is hereby incorporated by reference therein.

6. ☐ Microfiche Computer Program (Appendix)
7. Nucleotide and/or Amino Acid Sequence Submission
(if applicable, all necessary)
 - a. ☐ Computer Readable Copy
 - b. ☐ Paper Copy (identical to computer copy)
 - c. ☐ Statement verifying identity of above copies

ACCOMPANYING APPLICATION PARTS

8. ☐ Assignment Papers (cover sheet & document(s))
9. ☐ 37 CFR 3.73(b) Statement ☐ Power of Attorney
(when there is an assignee)
10. ☐ English Translation Document (if applicable)
11. ☐ Information Disclosure Statement (IDS)/PTO-1449 ☐ Copies of IDS Citations
12. ☐ Preliminary Amendment
13. ☒ Return Receipt Postcard (MPEP 503) (2)
(Should be specifically itemized)
14. ☐ Small Entity ☐ Statement filed in prior application,
Statement(s) Status still proper and desired
15. ☐ Certified Copy of Priority Document(s)
(if foreign priority is claimed)
16. ☐ Other:

17. If a CONTINUING APPLICATION, check appropriate box and supply the requisite information:

☐ Continuation ☐ Divisional ☐ Continuation-in-part (CIP) of prior application No: _____

18. CORRESPONDENCE ADDRESS

☒ Customer Number or Bar Code Label

21005

or ☐ Correspondence address below

(Insert Customer No. or Attach bar code label here)

NAME	James M. Smith, Esq.					
	HAMILTON, BROOK, SMITH & REYNOLDS, P.C.					
ADDRESS	Two Militia Drive					
CITY	Lexington	STATE	MA	ZIP CODE	02173	
COUNTRY	USA	TELEPHONE	(781) 861-6240	FAX	(781) 861-9540	

SIGNATURE

DATE

2/27/98

-1-

Date: 02/27/98 Express Mail Label No. EM482472756US

Inventors: Steven A. Bogen, Herbert H. Loeffler, and
John Purbrick

Attorney's Docket No.: CYL98-01

RANDOM ACCESS SLIDE STAINER WITH INDEPENDENT
SLIDE HEATING REGULATION

BACKGROUND OF THE INVENTION

5 Tissue sections or cellular monolayers are commonly
examined by microscopic examination, for both research and
clinical diagnostic purposes. Thin tissue sections or
cellular preparations are commonly 1 - 10 microns thick,
and are nearly transparent if untreated. In order to
visualize various histologic features, a wide array of
10 staining procedures have been developed over the years that
highlight various cellular or extracellular components of
the tissues. Histochemical stains, also commonly termed
"special stains," employ chemical reactions to color
various chemical moieties. Immunohistochemical stains
15 employ antibodies as probes to color specific proteins,
commonly via enzymatic deposition of a colored precipitate.
Each of these histochemical and immunohistochemical stains

09033376 022798

requires the addition and removal of reagents in a defined sequence for specific time periods, at defined temperatures. Therefore, a need arises for a slide stainer that can perform a diversity of stains simultaneously under
5 computer control, as specified by the technologist.

An early slide stainer for immunohistochemistry was described by David Brigati M.D., U.S. Patent 4,731,335. In that disclosure, microscope slides were closely apposed to each other, to form capillary gaps. The pairs of slides
10 were mounted in a holder that could be moved about by a mechanical arm along three axes. If slides were to be heated, all of the slides were moved as a group into a humidified heated chamber. Therefore, random access capability is not possible with this design.

15 In another slide stainer by Rogers and Sullivan, U.S. Patent 4,043,292, slides are mounted on a rotary carousel. Their invention heats the slides by passing a heated stream of air over the slides. All of the slides are heated to the same temperature.

20 Wooton, McLeod, and Read disclose another slide stainer that incorporates heat capability, in U.S. Patent 5,231,029. In that invention, a steam chamber is provided to heat slides. The humidity in the steam chamber is designed to be just below 100 percent. If the slides are
25 to be heated, they are placed into the chamber. Since the slides are either in or out of the chamber, all slides must be brought to the same heated temperature, a temperature approximately that of steam (100°C).

A recently described batch slide stainer
30 commercialized by Ventana Medical Systems, Inc. is

disclosed in U.S. Patent 5,595,707 by Copeland, et. al. In that disclosure, slides are placed on a rotary carousel that allows for the addition and flushing of reagents from the slide surface. Their slide stainer includes a heating
5 chamber that is heated by the introduction of warm air. A temperature sensor is contained within the chamber for providing temperature feedback to a microprocessor. Similar to the other slide stainers described above, all slides must be brought to the same temperature.

10 SUMMARY OF THE INVENTION

This invention relates to an improved slide staining device, for the application and removal of reagents to biologic tissue sections mounted on microscope slides. The improvement relates to the random access capability of the
15 slide stainer, i.e., one that performs any of a list of procedures to any of a plurality of biologic samples mounted on microscope slides. Since various procedures require heat at different times to enhance the rate of chemical reaction, a means has been developed to heat
20 slides to different temperatures, independently of the temperatures of other slides. This invention allows for heating each slide to its own specified temperature.

Any of the previously-described systems could potentially be modified to duplicate their heater control
25 systems to provide for multiple levels of heating control. For example, commercial thermal cyclers are now available that incorporate four different heating blocks that share the same microprocessor. However, the type of hard-wired temperature control mechanism that heats and cools four

different blocks would be expensive and cumbersome as the number of independent samples increases. For example, in the preferred embodiment of the present invention, forty-nine independent heating positions are described. If we assume that two wires provide power to the heater, and two wires provide temperature feedback from each heating sensor, then a total of 196 wires would need to be connected between the different heaters and the computer control circuitry. Placing all of these wires on a service loop between a stationary computer and a moving slide stainer presents yet another difficulty, increasing the cost of manufacture and servicing.

In accordance with one aspect of the invention, a moving plating, preferably a carousel, is adapted to support a plurality of microscope slides bearing biological samples. In particular, a plurality of flat heating stations are provided on the platform, each heating station supporting at least one microscope slide and, in a preferred embodiment, each heating surface supporting a single microscope slide. The heating stations are individually controlled to control temperatures to which the slides are heated.

According to another aspect of the invention, a plurality of heaters that can each heat at least one slide are associated with a moving platform that is adapted to support a plurality of microscope slides. Each heater includes a heating element set, each set having at least one heating element. A temperature controller electronic circuit mounted on the moving platform provides electrical power to the heating element such that each heating element

set can be heated to a different temperature. A user interface mounted off of the moving platform specifies the desired temperatures for the microscope slides through a communication link with the temperature controller electronic circuit.

Preferably, the communication link is a group of wires, the number of wires being fewer than the number of heating elements. To that end, the temperature controller electronic circuit may include a shift register which receives control data from the user interface, multiple shift registers of plural controllers being daisy chained. Individual temperature sensors may also be provided to provide temperature feedback information to the temperature controller electronic circuit.

15 BRIEF DESCRIPTION OF THE DRAWINGS

The foregoing and other objects, features and advantages of the invention will be apparent from the following more particular description of preferred embodiments of the invention, as illustrated in the accompanying drawings in which like reference characters refer to the same parts throughout the different views. The drawings are not necessarily to scale, emphasis instead being placed upon illustrating the principles of the invention.

25 FIG. 1 is a perspective view of a first embodiment of a slide stainer.

FIG. 2 is a top view of a slide frame for providing five sealed cavities above five different slides holding tissue samples.

2025 RELEASE UNDER E.O. 14176

FIG. 3 is a top view of a slide frame base.

FIG. 4 is a bottom view of a slide frame housing.

FIG. 5 is a top view of the slide frame housing with five microscope slides in their appropriate positions, 5 showing the area to which heat is applied.

FIG. 6 is a cross-sectional view of a slide frame resting on the slide rotor.

FIG. 7 is a schematic diagram of the heater and sensor wiring diagram, on the slide frame, and the interconnection 10 with the temperature controller.

FIG. 8 is a side cross-sectional view of a cartridge pump dispensing mechanism in the liquid dispensing and removal station.

FIG. 9 is a side cross-sectional view of a bulk liquid 15 dispensing station housed in the liquid dispensing and removal station.

FIGS. 10A and 10B are side cross sectional views of a vacuum hose and transport mechanism for removing liquid reagent and wash fluids from slides contained on the slide 20 rotor.

FIG. 11A is a side cross-sectional view of the aspiration head, showing its relationship to the glass slide in the slide frame.

FIG. 11B is a bottom en face view of the aspiration 25 head.

FIG. 12 is a perspective view of a second embodiment of a slide stainer.

FIG. 13 is a perspective view of the liquid handling zone of the second embodiment of the slide stainer.

352320"9432050

FIGS. 14A and 14B are side cross-sectional views of the liquid aspiration station of the second embodiment, with the aspiration head in the lowered (FIG. 14A) and raised (FIG. 14B) positions.

5 FIG. 15 is a schematic representation of the waste liquid pathways of the second embodiment.

FIG. 16 is a schematic representation of the bulk liquid dispense pathways of the second embodiment.

FIG. 17 is a schematic representation of the individual
10 heaters on the slide rotor and the temperature control boards mounted on the slide rotor.

FIG. 18 is a schematic diagram of the electronic circuitry of the temperature control board.

DETAILED DESCRIPTION OF THE INVENTION

15 FIG. 1 shows a first embodiment 1 of the invention in perspective view. Generally, the first embodiment 1 comprises a substantially circular assembly base 2, a slide rotor 3 rotatable on the assembly base 2, a reagent rotor 4 also rotatable on the assembly base, and a liquid
20 dispensing and removal station 5.

The slide rotor 3 is driven to rotate by a servo motor (not shown) and carries ten slide frames 6 that are radially asserted into and detachable from it. A top view of single slide frame 6 is shown in FIG. 2. Here,
25 positions for five slides, each with a tissue sample, are shown in positions 7a - 7e. The slide frame 6 comprises a slide frame base 8 shown in FIG. 3. The slide frame base 8 includes a heated area 9 which underlies each of the slide positions 7a - 7e and incorporates resistive heating

854220"923E050

elements, not shown. The heating elements are integrally formed in the slide frame base 8. Electricity for powering the heating elements is provided into the slide frame 6 from the assembly base 2 via first and second contacts 10.

5 Further, third and fourth contacts 11 enable temperature sensing of the heated areas via thermocouples also integrally formed in the slide frame base 8. In practice, a sum of three connectors are required, since contacts 10 and 11 share the same ground connection. Therefore, one of
10 the connectors 11 are left unused.

Adapted to overlay the slide frame base is a slide frame housing 12. FIG. 4 is a top view of the slide frame housing 12 showing essentially a rigid plastic or metal frame 13 with five oval holes 14a - 14e corresponding to
15 each of the slide positions 7a - 7e. A silicon rubber gasket 15 is also provided under the frame 13. Returning to FIG. 2, the slide frame housing 12, including the gasket 15 and frame 13, is bolted onto the slide frame base 8 by two Allen bolts 16 to provide individual sealed cavities
20 approximately 0.2 - 0.4 inches deep over each tissue sample slide placed at each of the slide positions 7a - 7e. As a result, a total of 3 ml of reagents and/or rinses can be placed in contact with the tissue samples of each one of the slides but a maximum quantity of 2 ml is preferable.
25 Since the silicon gasket 15 is compressed by the frame 13 against the microscope slides (not shown), the cavities over each of the frame positions are mutually sealed from each other.

FIG. 5 is a top view of a slide frame base 8 with five
30 microscope slides 17 in the positions denoted by 7a - 7e in

852220"9292E060

FIG. 3. The area of each slide 17 forming cavities, that are delimited by the silicone rubber gasket 15 and holes 14a - 14e is indicated by an approximately rectangular line 18, marking the chamber wall. The area denoted by the hatched bars indicates the area of the slide frame base 8 that includes heating elements 9. The entire heated area (hatched bars) is raised to the same temperature, bringing the group of five slides to the same desired temperature. The portion of each slide 17 that is not above the heated area does not generally bear a biologic tissue specimen. Rather, it is used for labeling purposes.

FIG. 6 is a cross-sectional view of an assembled slide frame base 8 and housing 12, collectively referred to previously as the slide frame 6. The microscope slide 17 is shown held in position, between the slide frame base 8 and housing 12. The slide frame 6 is resting on the slide rotor 3. In this view, the electrical connection between the slide frame 6 and an edge connector 19 is demonstrated. Four edge connectors per slide frame 6 are provided (contacts 10 and 11 in FIGS. 2 and 3). The electrical connection is fed from the edge connector 19 through the slide rotor via an insulated feed-through 20, to a terminal underneath the slide rotor 3. A wire then connects the terminal to a source of power or control circuitry (not shown).

FIG. 7 is a schematic diagram, showing two out of the ten heater 91 and sensor 92 circuits that can be placed on the instrument slide rotor. The heater is represented schematically as a resistive element, and corresponds to the heated area (hatched bars) of FIG. 5. Contacts 10 and

11 share a common ground connection, leaving one of the four connectors unused. Each of the circuits feeds into a temperature controller, represented schematically 21. Each slide frame sends three wires to the temperature controller 5 21 - - a heater power conductor 22, a sensor conductor 23, and a ground connection 24. The temperature controller 21 is mounted in a stationary position on the assembly base 2. Since the heaters and sensors are in frequent motion, they connect to the stationary temperature controller 21 via a 10 service loop (not shown). The service loop contains the wires from each of the edge connectors 19. Sufficient extra length is provided in the wires so that as the slide rotor rotates, the service loop travels around the slide rotor axis. The slide rotor 3 does not turn more than one 15 full revolution in either direction. The wires in the service loop are preferably bundled together with a wire tie, so that individual wires do not become entangled or caught underneath the slide rotor 3. Since there are three wires per circuit (wires 22 - 24), and there are ten slide 20 frames 6 on the slide rotor 3, the service loop contains a minimum of thirty wires.

Referring to FIG. 1, positioned above the slide rotor 3 is the reagent rotor 4. This reagent rotor is similarly adapted to rotate on the assembly base 2 and is driven by 25 another servo motor (not shown) under computer control (not shown). The reagent rotor 4 and the slide rotor 3 rotate independently of each other. The reagent rotor 4 is adapted to carry up to ten cartridge frames 25. Each of these cartridge frames 25 are detachable from the reagent 30 rotor 4 and can be selectively attached at any one of ten

06/22/98 09:33:05

-12-

1 The cartridge pump 46 is comprised of a liquid
reservoir 45 and the metering chamber 42. The liquid
reservoir 45 shown in this first embodiment 1 is a syringe
barrel. The metering chamber 42 is comprised of a
5 compressible elastomeric housing with a one-way inlet valve
(not shown) and a one-way outlet valve (not shown), both
valves aligned in a downwards direction of fluid flow.
When the hammer 26 compresses the metering chamber 42, the
liquid reagent contained within is ejected. When the
10 compressive force is removed, the negative pressure created
by the expansion of the elastomeric housing, trying to
resume its native, non-compressed shape, causes liquid to
flow inwards from the liquid reservoir 45. In this manner,
repetitive compression of the metering chamber 42 causes
15 repetitive dispensing of small aliquots of reagent.
Alternative cartridge pumps are presented in U.S. Patent
application Serial Number 08/887,178 filed July 2, 1997 and
U.S. Patent application Serial Number 09/020,983 filed
February 10, 1998 which are incorporated herein by
20 reference.

The dispensing station 5 further includes a means to
dispense liquids from a large bottle (FIG. 9). Bulk liquid
bottles 27 that can supply liquid into any one of the
microscope slides 17 on any one of the slide frames 6 via
25 rinse tubes 28. Each bulk liquid bottle 27 is connected to
its own rinse tube 28. The bulk liquid bottles 27 are
pressurized by a pump (not shown). The outflow tube (not
shown) from each bulk liquid bottle 27 passes through a
valve 47 that regulates the flow of liquid from that
30 bottle. By opening the valve for a defined period of time,

under computer control (not shown), with a defined pressure within the bottle 27, a known quantity of liquid can be dispensed onto the slide 17. The liquids placed within the bottles 27 are those that are used repeatedly among many
5 different procedures, such as water, saline, and alcohol.

As shown in FIG. 9, the bulk liquid bottles 27 are screwed into a female threaded cap 48 secured to the underside of the horizontal top wall 49 of the station frame. Compressed air from a compressor (not shown) is
10 provided to each bulk liquid bottle 27 through a pressure regulator 50. Tubing from the pressure regulator 51 transmits the compressed air to the inlet of the bulk liquid bottle 27. The pressure above the liquid enables the liquid to forced up through the dip tube 52 through the
15 rinse hose 53 when a pinch valve 47 is opened. Depending on the length of time that the pinch valve is opened, a pre-determined amount of liquid can be dispensed through the rinse tube 28.

The liquid dispensing and removal assembly 5 further
20 includes a liquid removal vacuum station, positioned adjacent to the rinse tubes 28 (not visible in FIG. 1). In order to remove liquid from the surface of a slide 17, the reagent rotor positions the slide at the liquid removal vacuum station, shown in a side cross-sectional
25 representation in FIGS. 10A and 10B. An external source of vacuum (not shown) is channeled through a trap flask 29, ultimately leading to a vacuum hose 30 that terminates in an aspiration head 31. The tubing connections are not shown in FIGS. 10A and 10B. The vacuum hose 30 and
30 aspiration head 31 are supported by a hose transport

98032300

mechanism 54 that allows the aspiration head 31 to be extended down into a cavity of a slide frame 6 to remove liquid covering the tissue sample on the slide 17. As the aspiration head contacts the liquid, the liquid is sucked upwards into the tubing and collected into the trap flask 29.

The vacuum hose transport mechanism 54 comprises a motor 32. A reciprocating link 33 is attached to a crank arm 34 so that the rotation of the motor 32 causes the reciprocating link 33 to traverse in a vertical direction. A bottom portion of the reciprocating link 33 is connected to a lever 55 that is pivotally attached to the station frame. The other end of this lever is connected to a vacuum hose clamp 35 that is connected via pivot arms 36 to a plate 37 rigidly attached to the station frame. The net effect of these connections is that when the motor 32 is rotated, the slide arm 33 descends in a vertical direction. Thus, the lever 55 is pivoted clockwise around its fulcrum causing the hose clamp 35 to pivot up and away on the two pivot arms 36 from the slide as shown in FIG. 10B. The motor is automatically turned off as the link 33 reaches its two extreme ends of movement by the contact of the electrical terminals 39 of the link to the contact plates 38 connected to the station frame.

25 The aspiration head 31 is shown in greater detail in
FIGS. 11A and 11B. FIG. 11A shows the aspiration head in a
lowered position, in cross-section, within the cavity
formed by the slide frame 6. The aspiration head 31
comprises a hollow interior manifold 40 through which the
30 vacuum force is transmitted across the entire lower surface

-15-

of the aspiration head 31. Eight holes 41 are drilled on the lower face of the aspiration head 31, through which the suction force is transmitted. Since the microscope slide 17 is planar, liquid on the slide surface spreads out in two dimensions. Therefore, in order to thoroughly remove liquid from all portions of the microscope slide 17, multiple aspiration sites are needed. We accomplish this with an aspiration head with a planar lower surface with multiple holes. The planar surface of the aspiration head 31 comes into close parallel apposition to the microscope slide 17. The aspiration head only contacts the liquid, not the microscope slide itself, lest it damage the glass slide 17 or the biologic specimen that it carries (not shown). Without such a design and only a single aspiration site, such as from a pipette, liquid distant from the aspirator would not be removed. Rather, it would cling to the distant surfaces of the glass slide 17, because of the surface tension on the glass. This would result in a residual volume of liquid that would otherwise be left on the surface of the slide 17. Having a close parallel apposition of the aspiration head is also helpful from the perspective of decreasing surface tension during liquid aspiration. The close parallel apposition of the bottom surface of the aspiration head with the microscope slide 17 creates a type of capillary gap. This gap helps to overcome surface tension, ensuring complete liquid removal.

A computer, not shown, controls the instrument functions. That is, an operator programs the computer with the information such as the location of reagents on the reagent rotor and the location of slides on the slide

10

30

accomplished in a somewhat similar liquid handling assembly (not shown) that is positioned in a liquid handling zone 65.

FIG. 13 shows the individual mechanisms contained within the liquid handling zone 65, including a hammer 66 for dispensing from cartridge pumps (not shown), an aspiration head 67 for removing liquid from the surface of slides, a bulk liquid dispensing port 68, and an air-mix head 69 for spreading and mixing liquids on the surface of a slide. The electromechanical mechanism for dispensing from cartridge pumps, by compressing a hammer 66 upon a metering chamber of a cartridge pump (not shown in FIG. 13), is similar to the previous embodiment (FIG. 8). Reagent dispensed from the cartridge pump (not shown) flows onto the slide by passing through a roughly rectangular hole in the platen 64.

The aspiration head 67 also functions in a similar manner to that of the previous embodiment. In order to simplify the linkage mechanism for lowering and raising the head 67, the head moves solely in a vertical direction. This is shown in further detail in FIGS. 14A and 14B. FIG. 14A shows a side cross-sectional view of the aspiration head in a down position, within a cavity formed by the microscope slide 75 (bottom surface) and a slide chamber clip 76 (lateral walls). As in the first embodiment, a gasket (not shown) seals the surface where the slide chamber clip 76 contacts the microscope slide 75. A linear stepper motor 73 moves the aspiration head up and down, under computer control (demonstrated schematically in FIG. 15). As in the first embodiment 1, the aspiration head 67

comprises a hollow manifold 74 connected to a source of vacuum. Eight holes communicate between the bottom of the aspiration head 67 and the exterior, through which liquid is aspirated. When vacuum is supplied to the aspiration head 67, and the head 67 is lowered adjacent to the slide, the liquid reagent on top of the slide is aspirated off and collected in a trap bottle 59 (shown schematically in FIG. 15). When the aspiration head 67 is not in use, it is raised to the up position (FIG. 14B), allowing free rotation of the slide rotor 77.

FIGS. 14A and 14B also show the physical location of a heating element 78, represented as a resistive element inside a rectangular box with cross-hatched lines. Each slide rests directly on the heating element 78, so that heat is directly communicated to the microscope slide. A thermistor is incorporated into each heating element (not shown in FIGS. 14A and 14B). Each of forty-nine microscope slides 75 has its own heating element 78, so that the temperature of each slide 75 can be independently regulated. Power for the heating element 78 is supplied directly from a temperature control board 79 that is affixed to the underside of the slide rotor 77. Seven identical temperature control boards 79 are so mounted underneath the slide rotor 77, evenly spaced around the periphery. Each temperature control board supplies power for seven heating elements 78. The means by which this is accomplished is explained later, in reference to FIGS. 17 and 18.

An important aspect of this embodiment, not highlighted in the previous embodiment 1, is the provision for the

segregation of waste liquids that are removed from the surface of the slide. A schematic diagram explaining how this is accomplished is shown in FIG. 15. Three different waste bottles 59 are mounted on the instrument.

5 Connections 70 are also provided on the instrument for a large external trap bottle 71, typically of a ten or twenty liter capacity for aqueous waste. Four solenoid valves, labelled 80A - 80D control to which bottle aspirated liquid will be directed. These valves are under computer control,
10 schematically represented by the box labelled "controller" 86. Valve 81 is a three way valve. It can allow a direct connection between the vacuum pump 82 and the overflow trap 83, or between the pump and the ambient environment. A connection to the ambient environment is required if the
15 aspiration system needs to be bypassed when the air-mix head 69 is in use. If valves 80A and 81 are appropriately opened, the pump 82 turned on, and the aspirator head 67 lowered so as to aspirate liquid, the liquid will be directed upwards into the tubing, as represented by the
20 arrow "fluid flow." Liquid will then follow the only path available, and be collected into the external trap bottle 71. Valves 80B - 80D function similarly for their respective trap bottles 59. A small overflow trap bottle 83 is also inserted into the line with its own fluid sensor
25 93. This provision is included so as to detect if any of the trap bottles 59, or external trap bottle 71 are overflowing with waste liquid. In that case, liquid would enter the overflow trap bottle and be detected by the fluid sensor. That information would be communicated to the

980320-9232050

controller 86, which would shut the system down and alert the instrument operator on the computer screen.

Referring to FIG. 13, the liquid handling zone also includes an air-mix head 69. A schematic representation of the air flow into the air-mix head 69 is shown in FIG. 15. The pump generates a high velocity air stream that is channeled into the air-mix head 69. Air intake to the pump is via the three way solenoid valve 81 (FIG. 15). The solenoid valve 81 (FIG. 15) switches so as to channel air directly from the atmosphere to the pump (FIG. 15), bypassing the aspiration system and trap bottles 59 and 71. The high velocity air flow is focused onto the slide. The air-mix head 69 travels back and forth along the length of the slide, pushed and pulled by a belt and pulley that is attached to a motor (not shown). The net effect of this system is to direct a curtain of air back and forth along the length of the slide, causing liquid to be mixed and spread along the surface of the microscope slide.

The liquid handling zone 65 (FIG. 12) includes a bulk liquid dispensing port 68 (FIG. 13). The function of the rinse tubes 28 of the first embodiment 1 (shown in FIG. 1) are all incorporated into a single bulk liquid dispensing port 68 in this preferred embodiment. Therefore, slides are positioned under the bulk liquid dispensing port 68 regardless of the bulk liquid bottle that the liquid is actually derived from. A schematic representation of the fluid pathways and control valves is shown in FIG. 16. The bulk liquid bottles 57 are each connected to a source of pressure, that is generated by a pump 85. The pressure is communicated to the bulk liquid bottles 57 via a pressure

manifold 94. Solenoid valves 72a - 72f are placed between the bulk liquid dispensing port 68 and each bulk liquid bottle 57. Liquid flows out the bulk liquid dispensing port 68 only when one or more of the valves 72a - 72f are open. A pressure switch 84 also communicates with the pressure manifold 94. It is capable of sensing the amount or pressure contained within the manifold 94. When it falls below a specified level, it communicates with the controller 86 causing activation of the pump 85. As the pump generates an increased amount of air pressure within the pressure manifold, the pressure switch resets, causing the pump to stop pumping. In this manner, a relatively constant pressure head is maintained within the pressure manifold 94.

A dispense sensor 95 is positioned underneath the bulk liquid dispensing port 68 to provide verification that liquid was dispensed when one of the solenoid valves 72a - 72f were transiently opened. The dispense sensor 95 comprises an optical sensor and an LED light source. When liquid is dispensed from the bulk liquid dispensing port 68, the liquid interrupts the light beam. The change in resistance across the sensor as a result of the decrement in light intensity is communicated to the controller 86.

This second, preferred embodiment of the invention includes the capability to independently heat the forty-nine slides to different temperatures. A novel aspect of this embodiment is the method for independently regulating the amount of power that each of the forty-nine heaters receives. Moreover, each heater also incorporates a temperature sensor. Each of these sensors must

communicate with the computer 86 in order to allow for appropriate temperature feedback and regulation. In the first embodiment 1, groups of up to five slides were under a single, common temperature control mechanism. Each heating group had wires that directly connected with the temperature controller (FIG. 7). With three wires per group (power for heat, sensor feedback, and a shared ground) and ten groups of slides, at least thirty wires were contained in the service loop. If a similar system were used for forty-nine different heaters, as in this preferred embodiment, 147 wires would be required in the service loop. Such a bulky service loop would be problematic. Therefore, an alternative method is developed in this preferred embodiment.

FIG. 17 shows the relationship between each of the heating elements 78 mounted on the slide rotor 77, depicting the heating element 78 as a resistive element. A single sensor 87 is adjacent to each heater. The combination of a single heating element 78 and sensor 87 are so positioned so as to provide a location 88 for a single slide to be heated. The physical layout of this location 88 is demonstrated in FIGS. 14A and 14B. Two wire leads from each heating element 78, and two wire leads from each sensor 87 are connected directly to a temperature control board mounted on the slide rotor 77. Each temperature control board is capable of connecting to up to eight different heater and sensor pairs. Since this embodiment incorporates forty-nine slide positions, seven boards 79 are mounted to the underside of the slide rotor, each connecting to seven heater-sensor pairs. One

heater-sensor position per temperature controller board 79 is not used. Also shown in FIG. 17 is the serial connection 89 of each of the seven temperature control boards, in a daisy-chain configuration, by six wires. The first temperature control board is connected via a service loop 90 to the computer 86. The service loop contains only six wires tied together in a harness.

FIG. 18 is an electronic schematic diagram of the temperature control board 79. The design of the temperature control board 79 was driven by the need to minimize the number of wires in the flexible cable (service loop 90) between the heaters and the computer. To minimize the length of wires, seven temperature controller boards 79 are used, each mounted on the slide rotor. Thus, each heater is positioned close to its associated electronics and the size of each board 79 is kept small because each runs only seven heating elements 78. Each temperature controller board 79 includes the function of an encoder and decoder of temperature data. That data relates to the actual and desired temperature of each of heating elements 78. The data flows back and forth between the computer 86 and the temperature control board 79. If an individual heating element 79 requires more or less heat, the computer communicates that information to the temperature control board 79. The temperature control board 79, in turn, directly regulates the amount of power flowing to each heater. By placing some of the logic circuitry on the slide rotor, in the form of the temperature control boards 79, the number of wires in the service loop 90 , and their length, are minimized.

In this embodiment, the temperature control board 79 system was designed as a shift register. The machine's controlling microprocessor places bits of data one at a time on a transmission line, and toggles a clock line for each bit. This causes data to be sent through two shift register chips on each control board, each taking eight bits. There are thus 16 x 7 or 112 bits to be sent out. Referring to FIG. 18, the data comes in on connector J9.1, and the clock line is J9.2. The shift registers used in this design are "double buffered," which means that the output data will not change until there is a transition on a second clock (R clock), which comes in on pin J9.3. The two clocks are sent to all seven boards in parallel, while the data passes through the shift register chips (U1 and U2) on each board and is sent on from the second shift register's "serial out" pin SDOUT to the input pin of the next board in daisy chain fashion. It will be seen that a matching connector, J10, is wired in parallel with J9 with the exception of pin 1. J10 is the "output" connector, which attaches via a short cable to J9 of the next board in line, for a total of seven boards. The other three pins of J9 are used for power to run the electronics (J9.4), electronic ground (J9.5), and a common return line (J9.6) for temperature measurement function from the sensors.

Of the sixteen data bits sent to each board, eight control the on/off status of up to eight heating elements 78 directly. This can be accomplished with a single chip because shift register U2 has internal power transistors driving its output pins, each capable of controlling high power loads directly. Four of the remaining eight bits are

Temperature sensing is accomplished by a voltage divider technique. A thermistor 87 and a fixed resistor (5.6 kilohms, R1 - R8, contained in RS1) are placed in series across the 5 volt electronic power supply. When the thermistor is heated, its resistance drops and the voltage

at the junction point with the 5.6 kilohm resistor will drop.

There are several advantages to the design used in this embodiment. Namely, the temperature control boards 79 are
5 small and inexpensive. Moreover, the heater boards are all identical. No "address" needs to be set for each board 79. Lastly, the service loop 90 is small in size.

An alternative potential design is that each temperature control board 79 could be set up with a
10 permanent "address" formed by adding jumper wires or traces cut on the board. The processor would send out a packet of data which would contain an address segment and a data segment, and the data would be loaded to the board whose address matched the address sent out. This approach takes
15 less time to send data to a particular board, but the address comparison takes extra hardware. It also demands extra service loop wires to carry the data (if sent in parallel) or an extra shift register chip if the address is sent serially. As yet another potential design is that
20 each temperature control board 79 could have its own microprocessor. They could all be connected via a serial data link to the main computer 86. This approach uses even fewer connecting wires than the present embodiment, but the cost of hardware is high. It also still implies an
25 addressing scheme, meaning that the boards would not be identical. Also, code for the microprocessors would be required.

EQUIVALENTS

10

CLAIMS

What is claimed is:

1. A microscope slide stainer with random access slide staining capability, comprising:
- 5 a moving platform adapted to support a plurality of microscope slides bearing biologic samples;
- a plurality of heating element sets, each set having at least one heating element and each set heating at least one slide, each of said heating
- 10 element sets having the capability of heating to different temperatures;
- a temperature controller electronic circuit that provides electrical power to said heating element sets, said temperature controller being mounted on the moving
- 15 platform; and,
- a user interface in communication with the temperature controller electronic circuit and through which a desired temperature for microscope slides is specified, said user interface being mounted off of the
- 20 moving platform.
2. A microscope slide stainer as claimed in claim 1, wherein the temperature controller, capable of moving on said moving platform, and the user interface, not mounted on said moving platform, communicate
- 25 electrically via a group of wires.

00326-02798
86429-922060

3. A microscope slide stainer as claimed in claim 2,
wherein the number of wires in the group of wires is
fewer than the number of heating element sets.
4. A microscope slide stainer as claimed in claim 1,
5 wherein the temperature controller electronic circuit
comprises a shift register which receives control data
from the user interface.
5. A microscope slide stainer as claimed in claim 1,
further comprising a temperature sensor for providing
10 temperature feedback information to the temperature
controller electronic circuit.
6. A microscope slide stainer as claimed in claim 1
wherein each heating element set heats a single slide.
7. A microscope slide stainer as claimed in claim 1
15 wherein each heating element set comprises a flat slide
support surface.
8. A microscope slide stainer with random access slide
staining capability, comprising:
a plurality of microscope slides bearing biologic
20 samples, positioned on a moving platform;
a plurality of heating element sets on the moving
platform, each set having at least one heating element
and each set capable of heating at least one slide,
each capable of heating to a temperature distinct from
25 the temperature of other heaters;

2025-09-29 14:22:29

35/220-926060

5 a user interface through which a desired temperature for each microscope slide is specified, said user interface being mounted off of the moving platform and said user interface comprising electronic circuitry; and,

10 a group of wires, for providing an electrical connection between the heating elements on the moving platform and the user interface, the number of wires in said group of wires being less than the number of heater element sets.

9. A microscope slide stainer as claimed in claim 8, further comprising a temperature sensing means for providing temperature feedback data to said user interface.

15 10. An automated device for preparation or incubation of biologic samples, comprising:

a moving platform adapted to support a plurality of biologic samples;

20 a plurality of heaters positioned on the moving platform so as to provide heat to one or more samples;

a computer that specifies the desired temperature for each heater, said computer being mounted off of the moving platform;

25 independent heating control to each of said heaters, said heating control comprising:

a plurality of temperature controller electronic circuits mounted on the moving platform, each supplying electrical power to at least one heater; and

5

- 10

15

20

25

interface means being mounted off of the moving platform.

RANDOM ACCESS SLIDE STAINER WITH INDEPENDENT
SLIDE HEATING REGULATION

An automated slide stainer with slides mounted in a horizontal position on a rotary carousel. Reagents and rinse liquids are automatically dispensed onto tissue sections or cells mounted on slides for the purpose of performing chemical or immunohistochemical stains. The rinse liquids are removed by an aspiration head connected to a source of vacuum. Individual slides or groups of slides are supported on flat heating stations for heating to individual temperatures. Temperature control electronics on the carousel are controlled by a user interface off of the carousel.

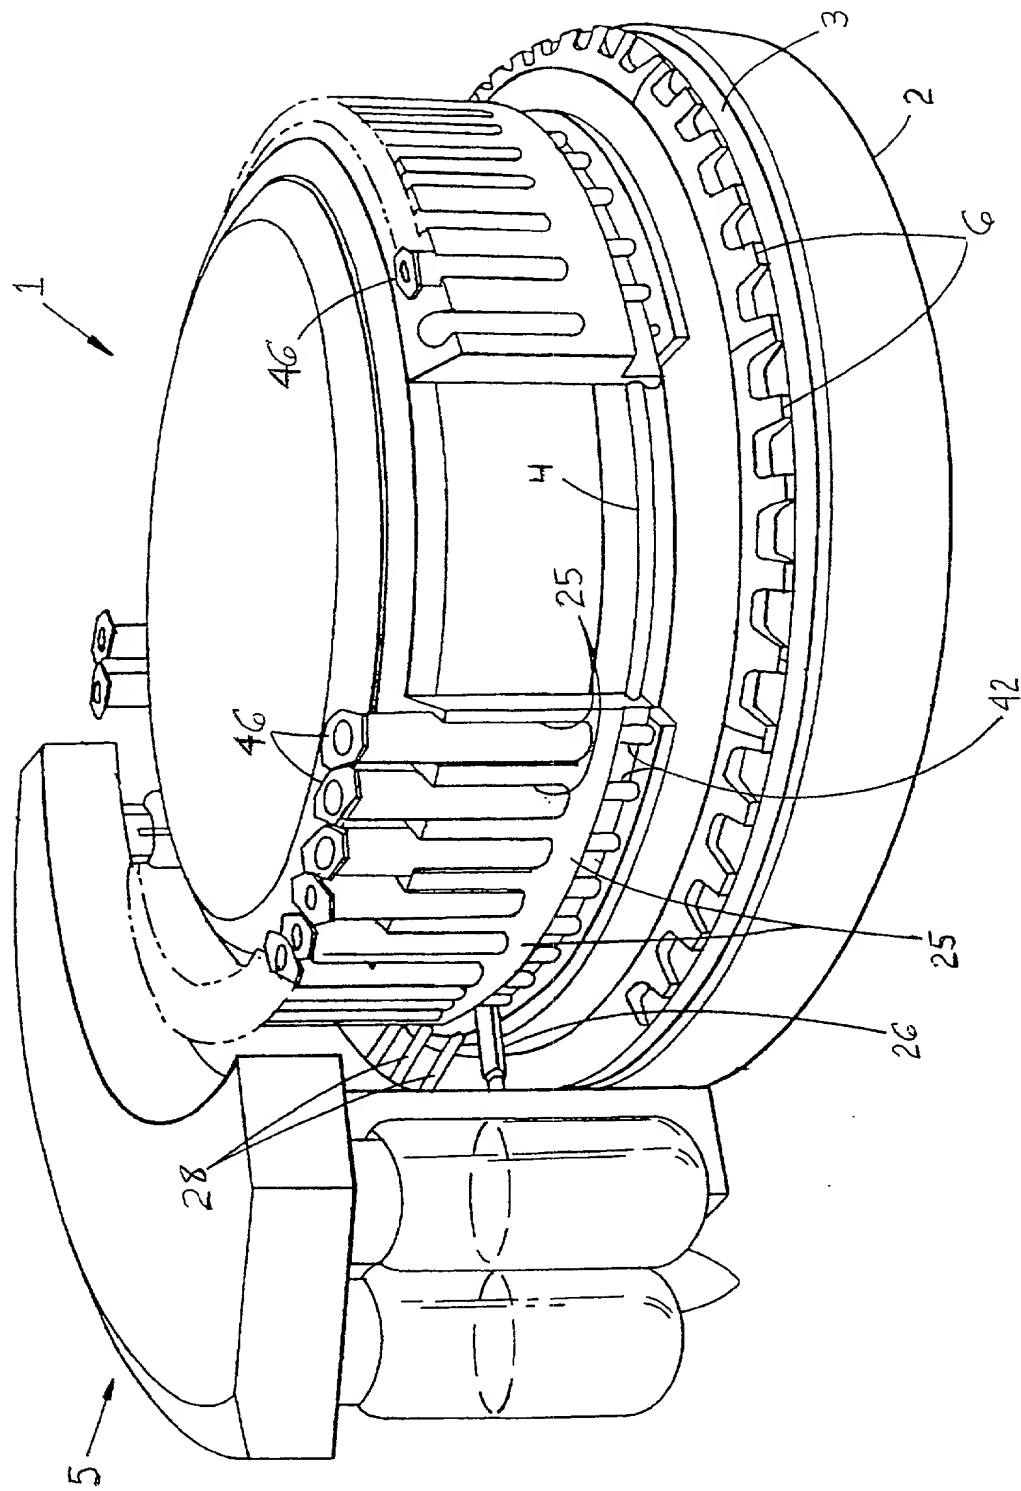


FIG. 1

FIG. 2

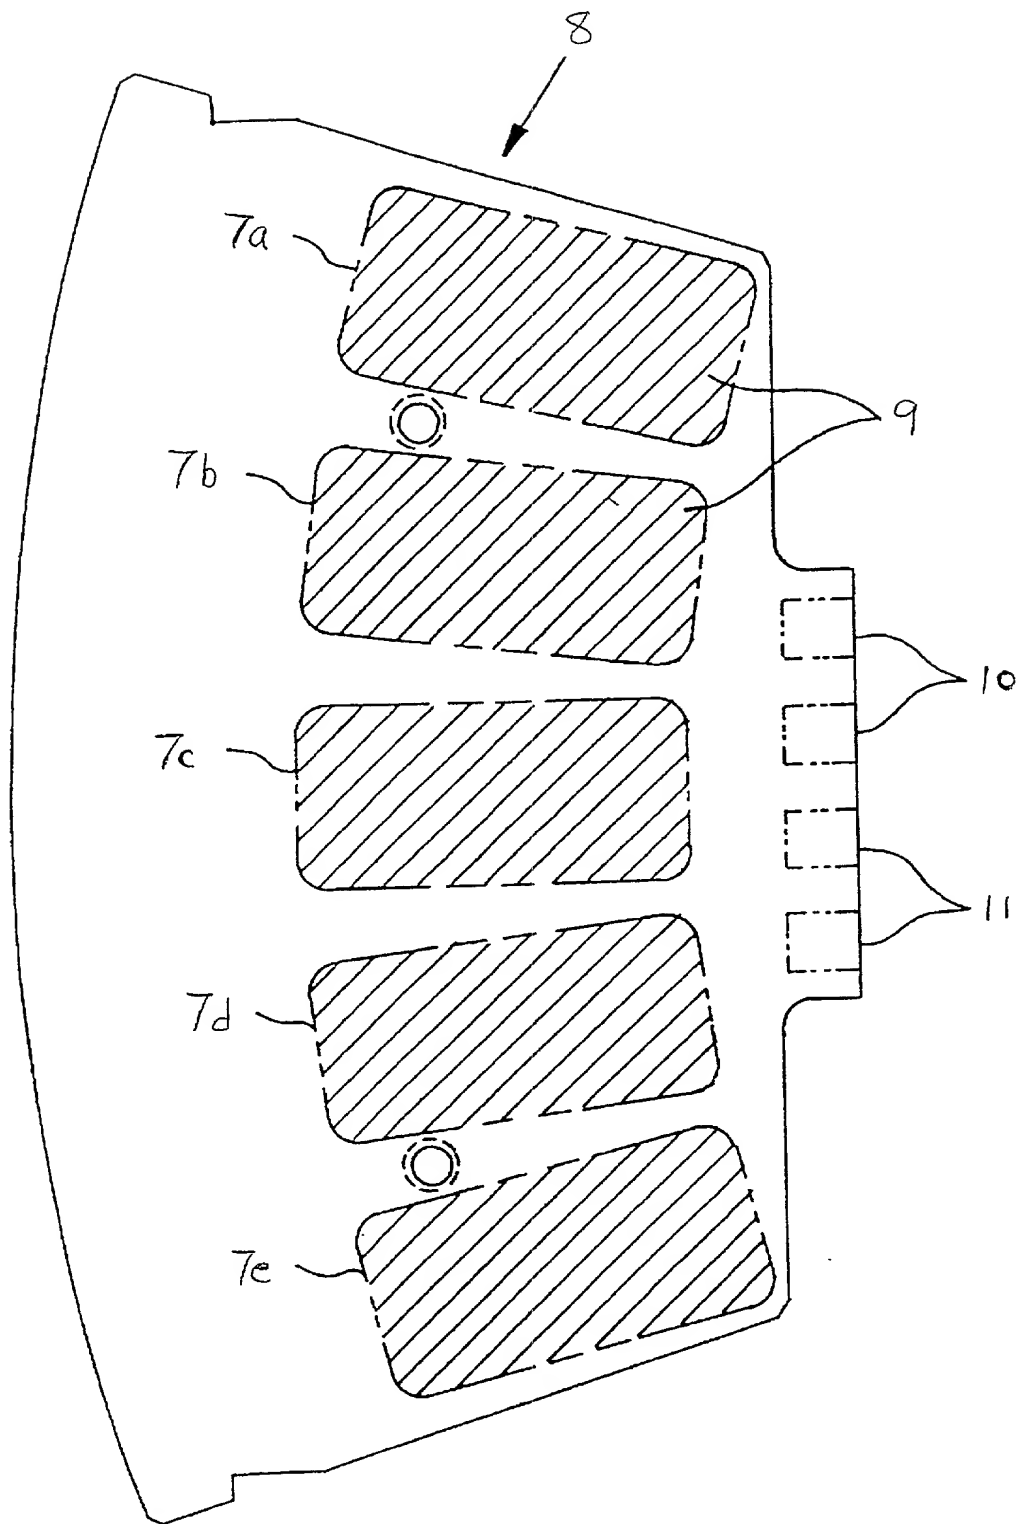


FIG. 3

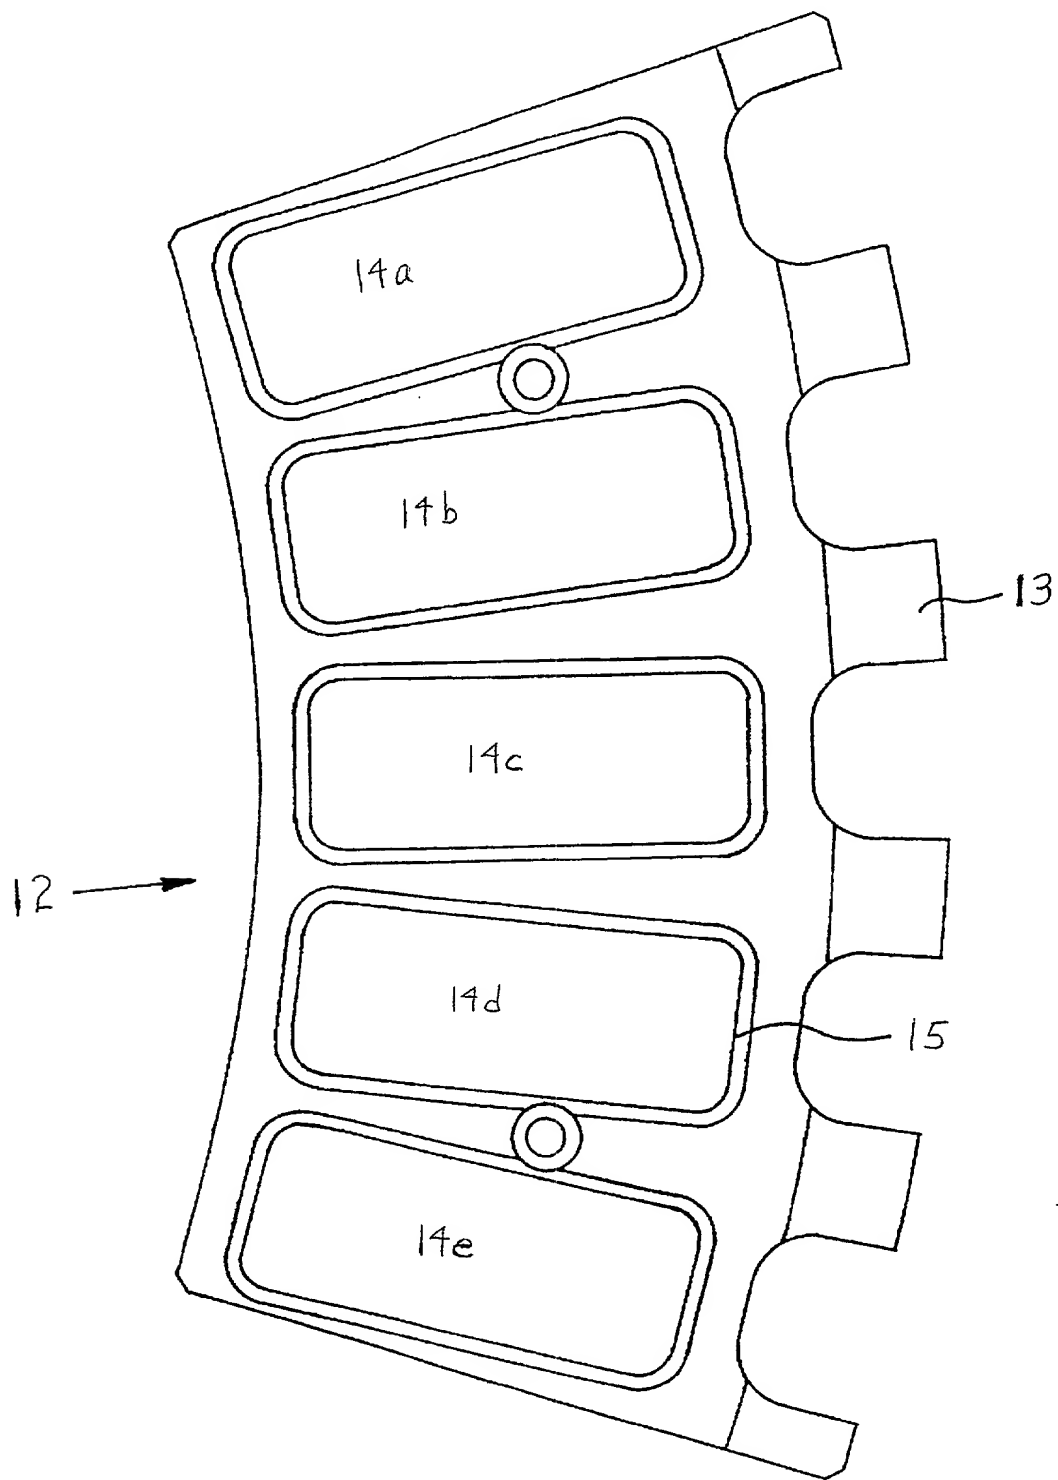


FIG. 4

864220-9292050

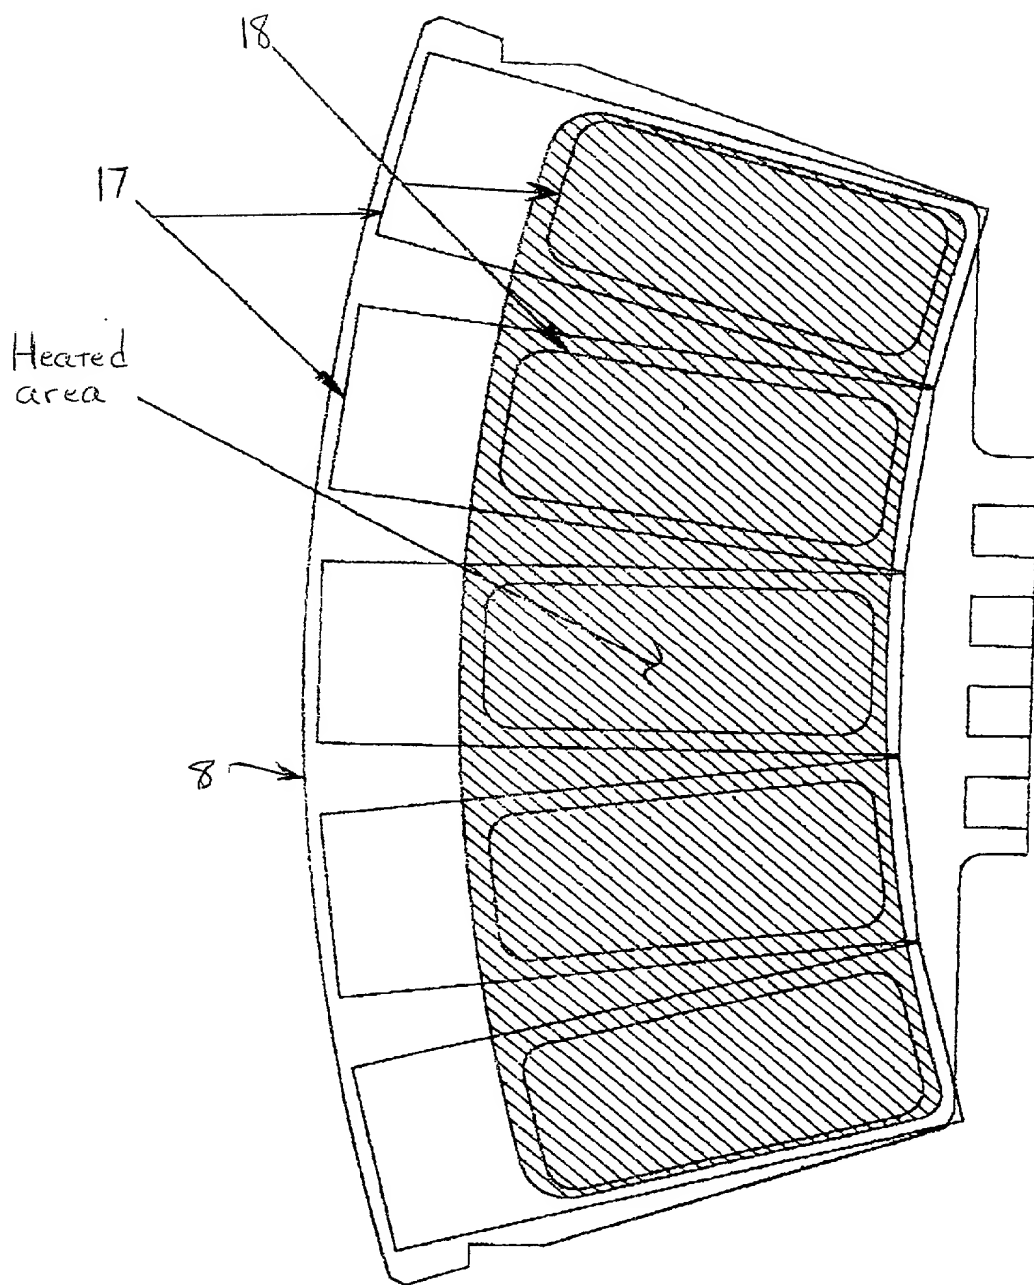


FIG. 5

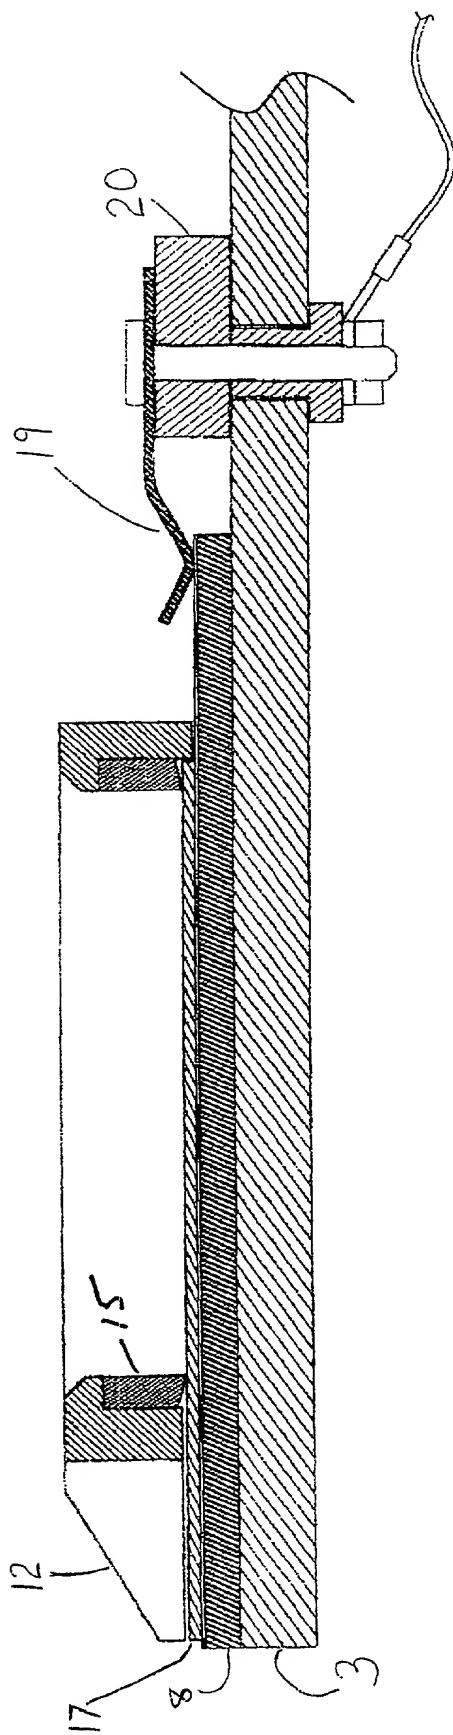


FIG. 6

The diagram illustrates a temperature control system for a semiconductor device. The device is shown as a complex structure with various components labeled:

- HEATER 91**: A zigzag line representing a heater element.
- SENSOR 92**: A circle representing a temperature sensor.
- 10**: A series of small squares representing a contact or interface.
- 11**: A series of small squares representing a contact or interface.
- 22**: A vertical line representing a connection or interface.
- 23**: A vertical line representing a connection or interface.
- 24**: A ground symbol.

The system is connected to a **TEMPERATURE CONTROLLER 21**, which is shown as a large rectangular block. The controller has several input/output lines:

- HEAT 1**: A line connecting the heater 91 to the controller.
- SENSE 1**: A line connecting the sensor 92 to the controller.
- HEAT 2**: A line connecting the heater 91 to the controller.
- SENSE 2**: A line connecting the sensor 92 to the controller.

The controller is powered by a **POWER** source, indicated by an arrow pointing to the bottom of the block.

FIG. 7

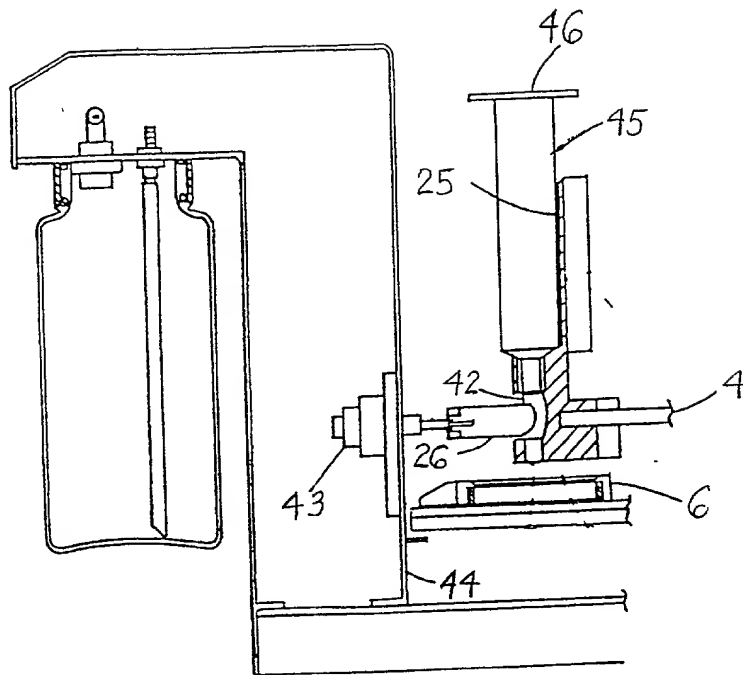


FIG. 8

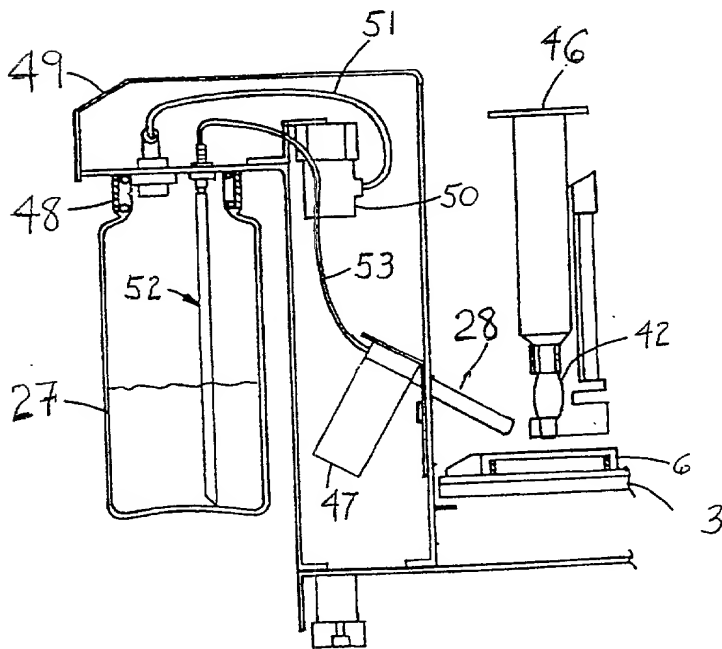


FIG. 9

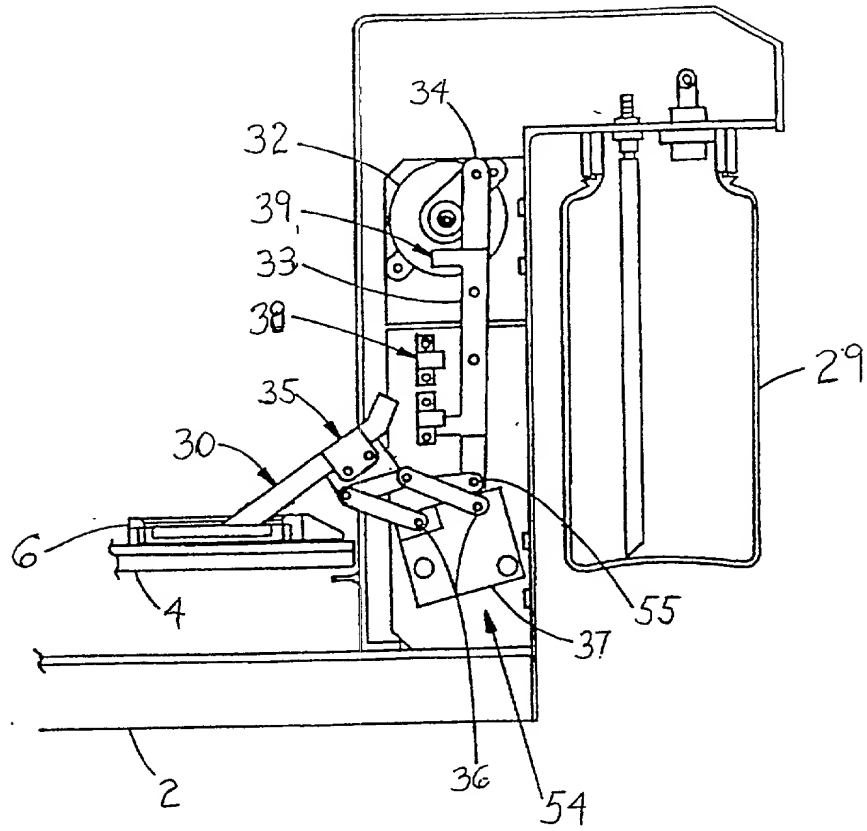


FIG. 10A

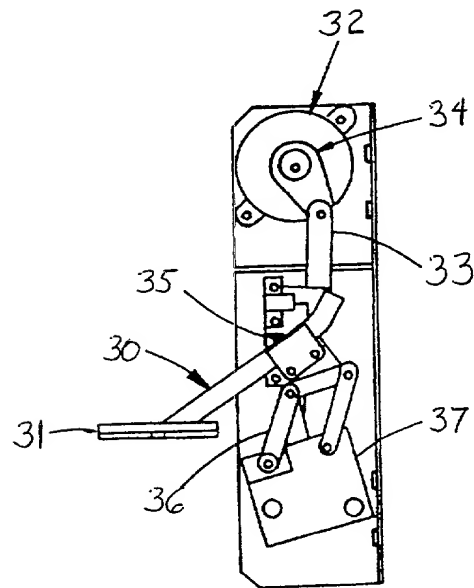


FIG. 10B

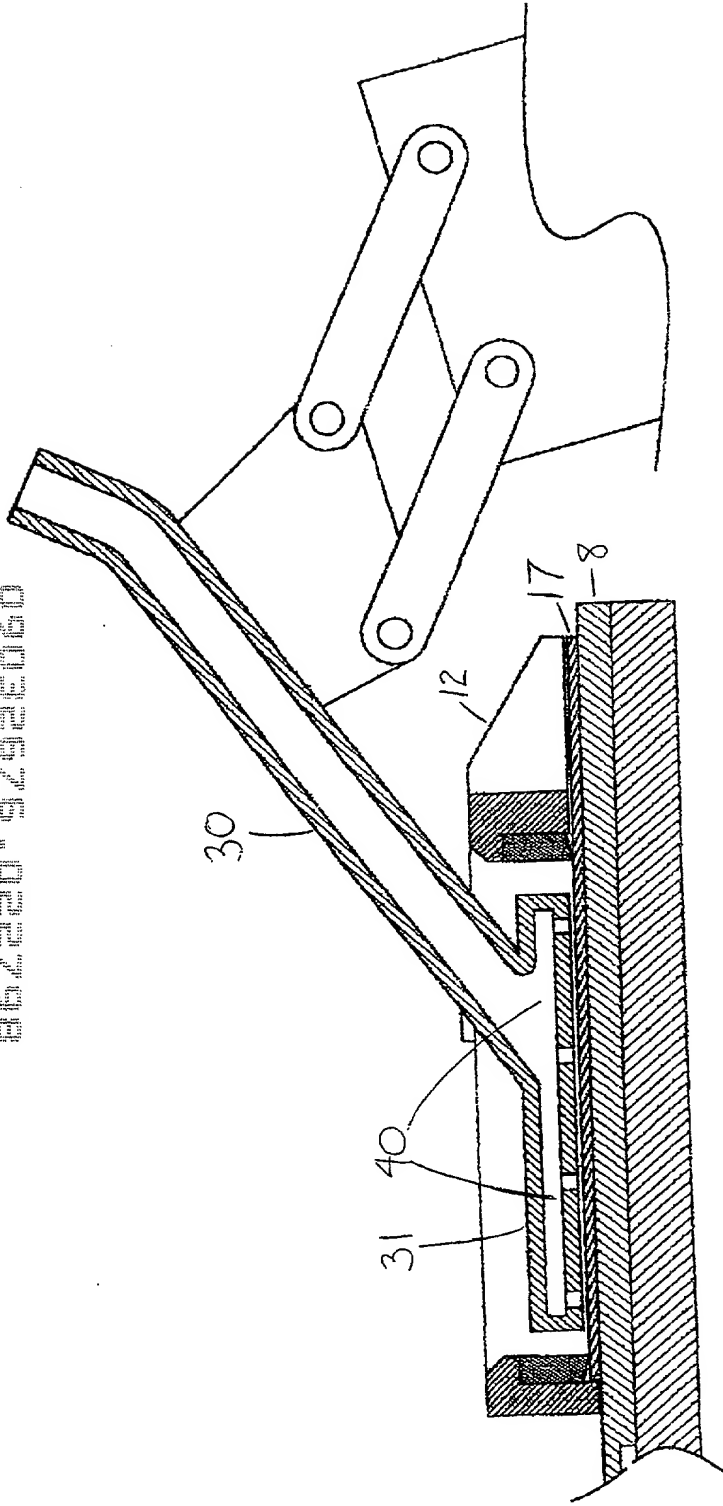


FIG. 11A

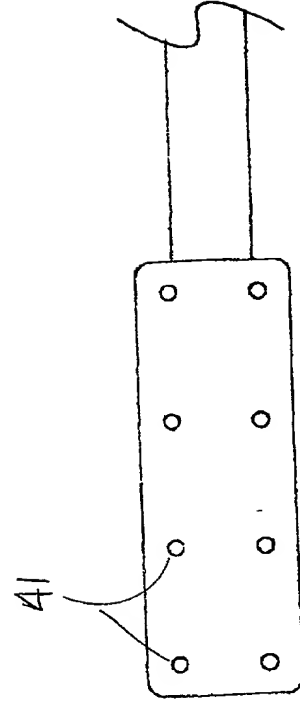


FIG. 11B

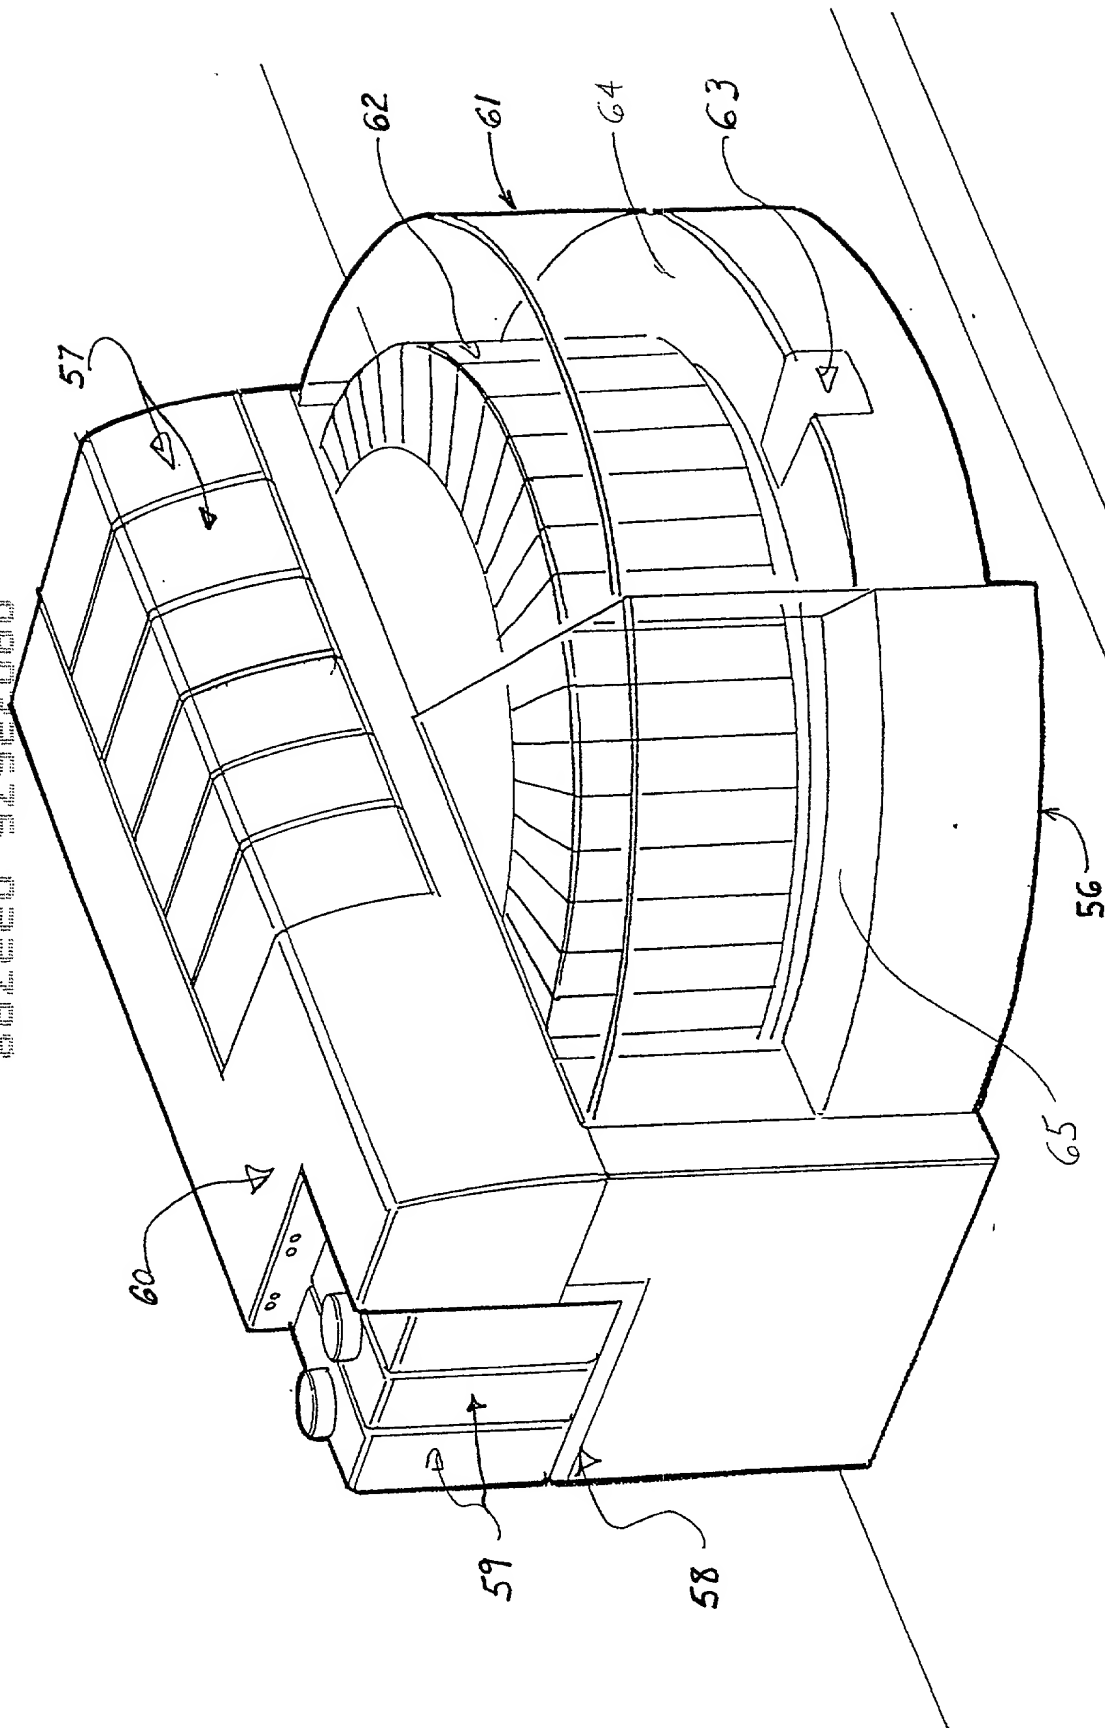


FIG. 12

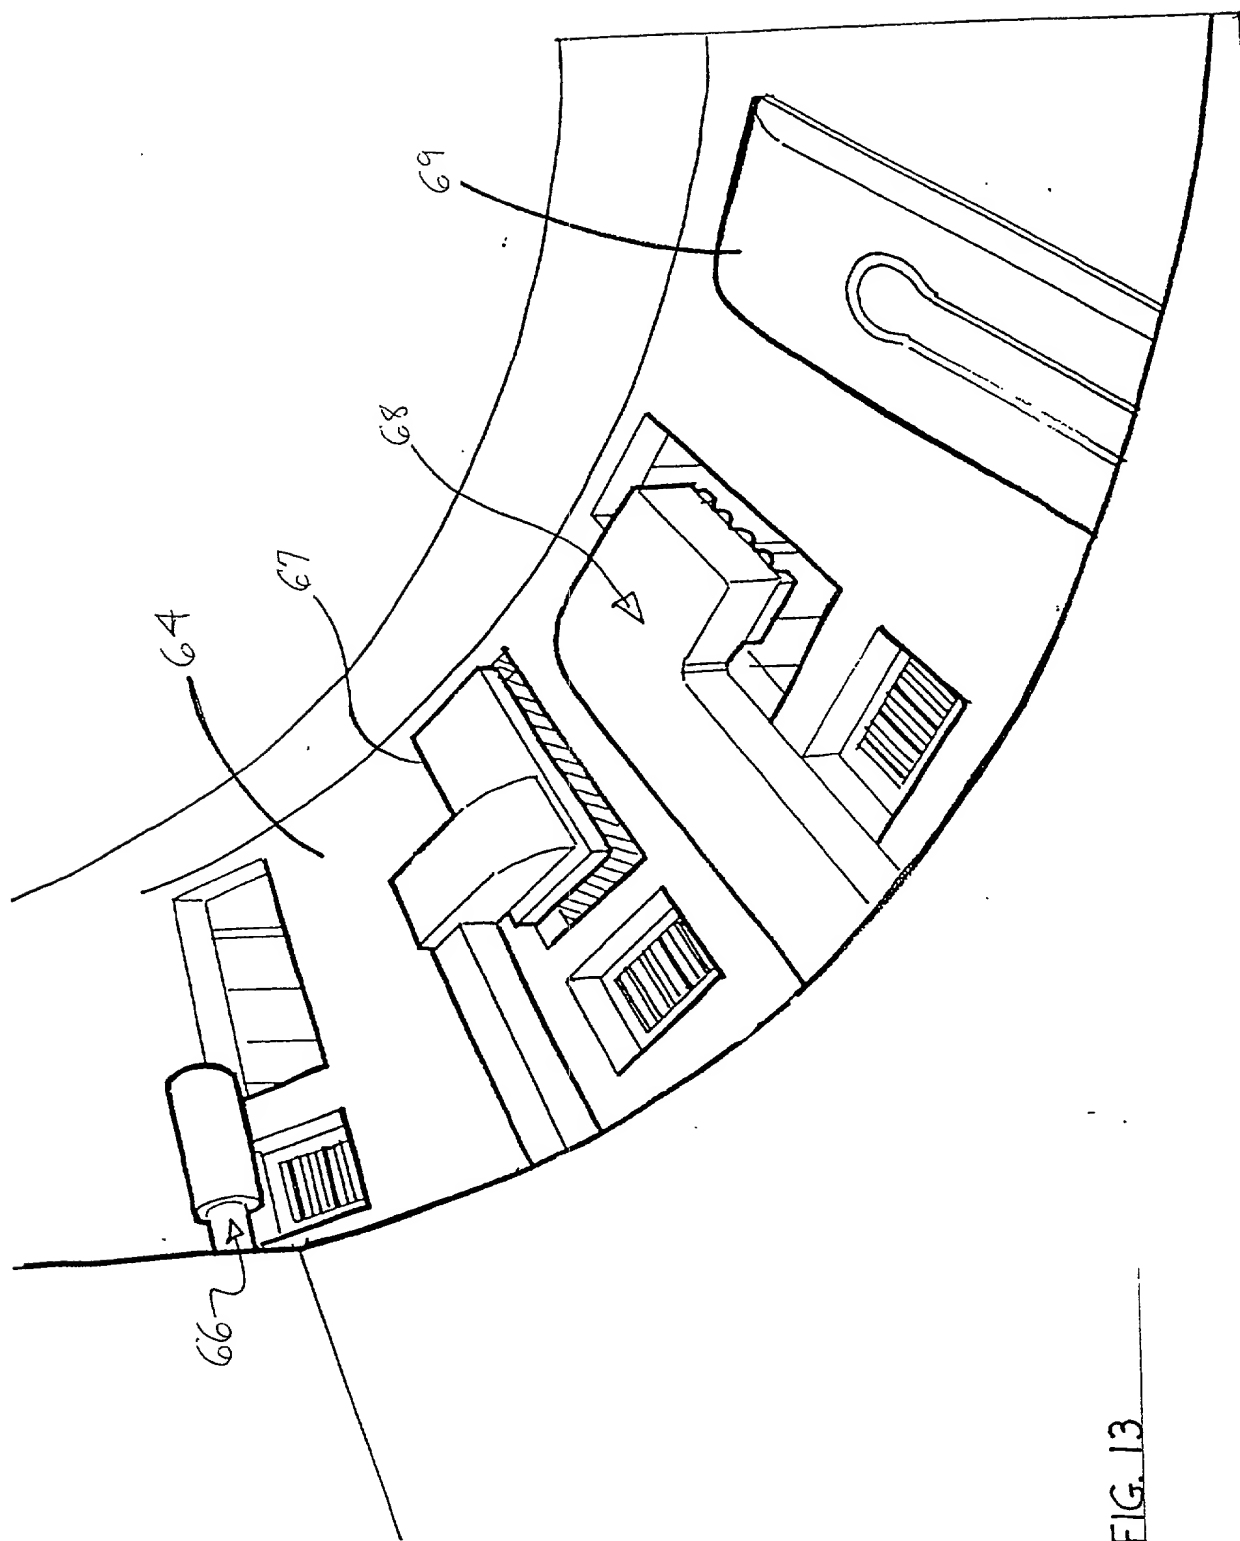


FIG. 13

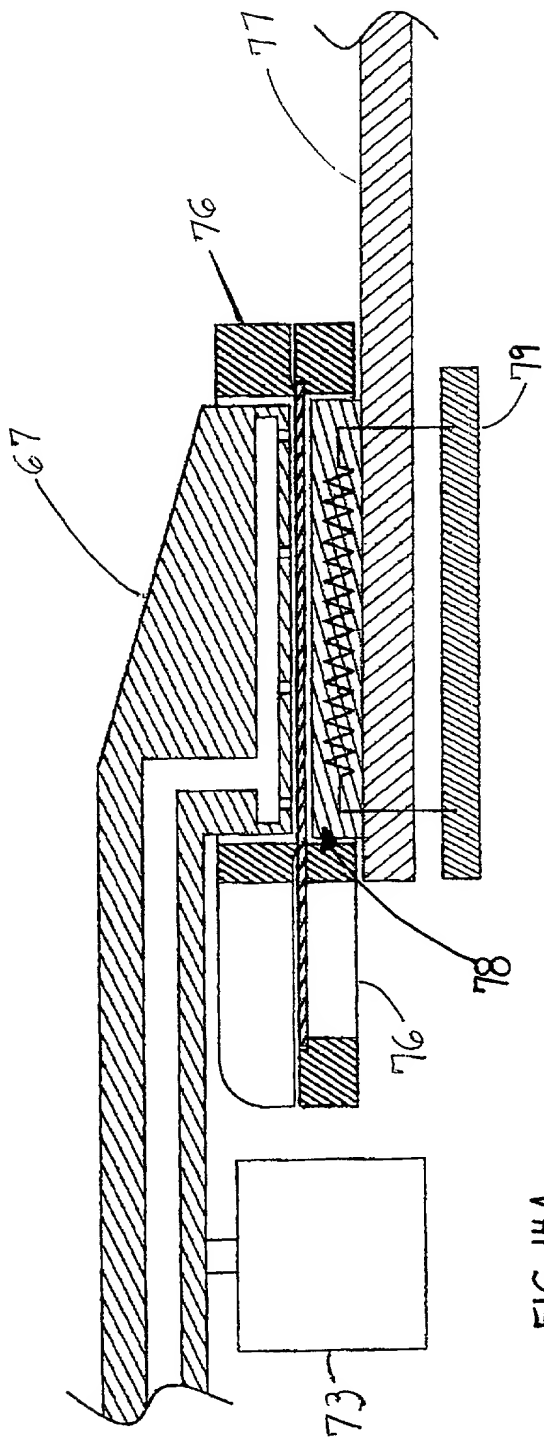


FIG. 14A

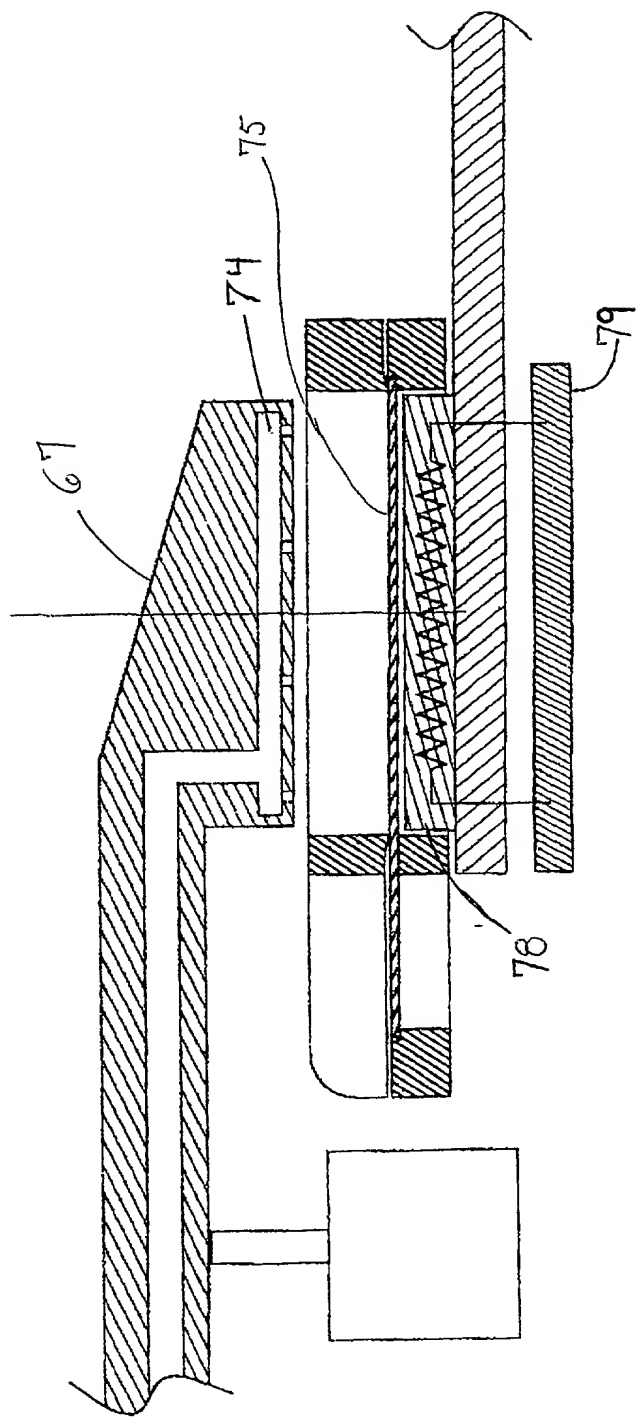


FIG. 14B

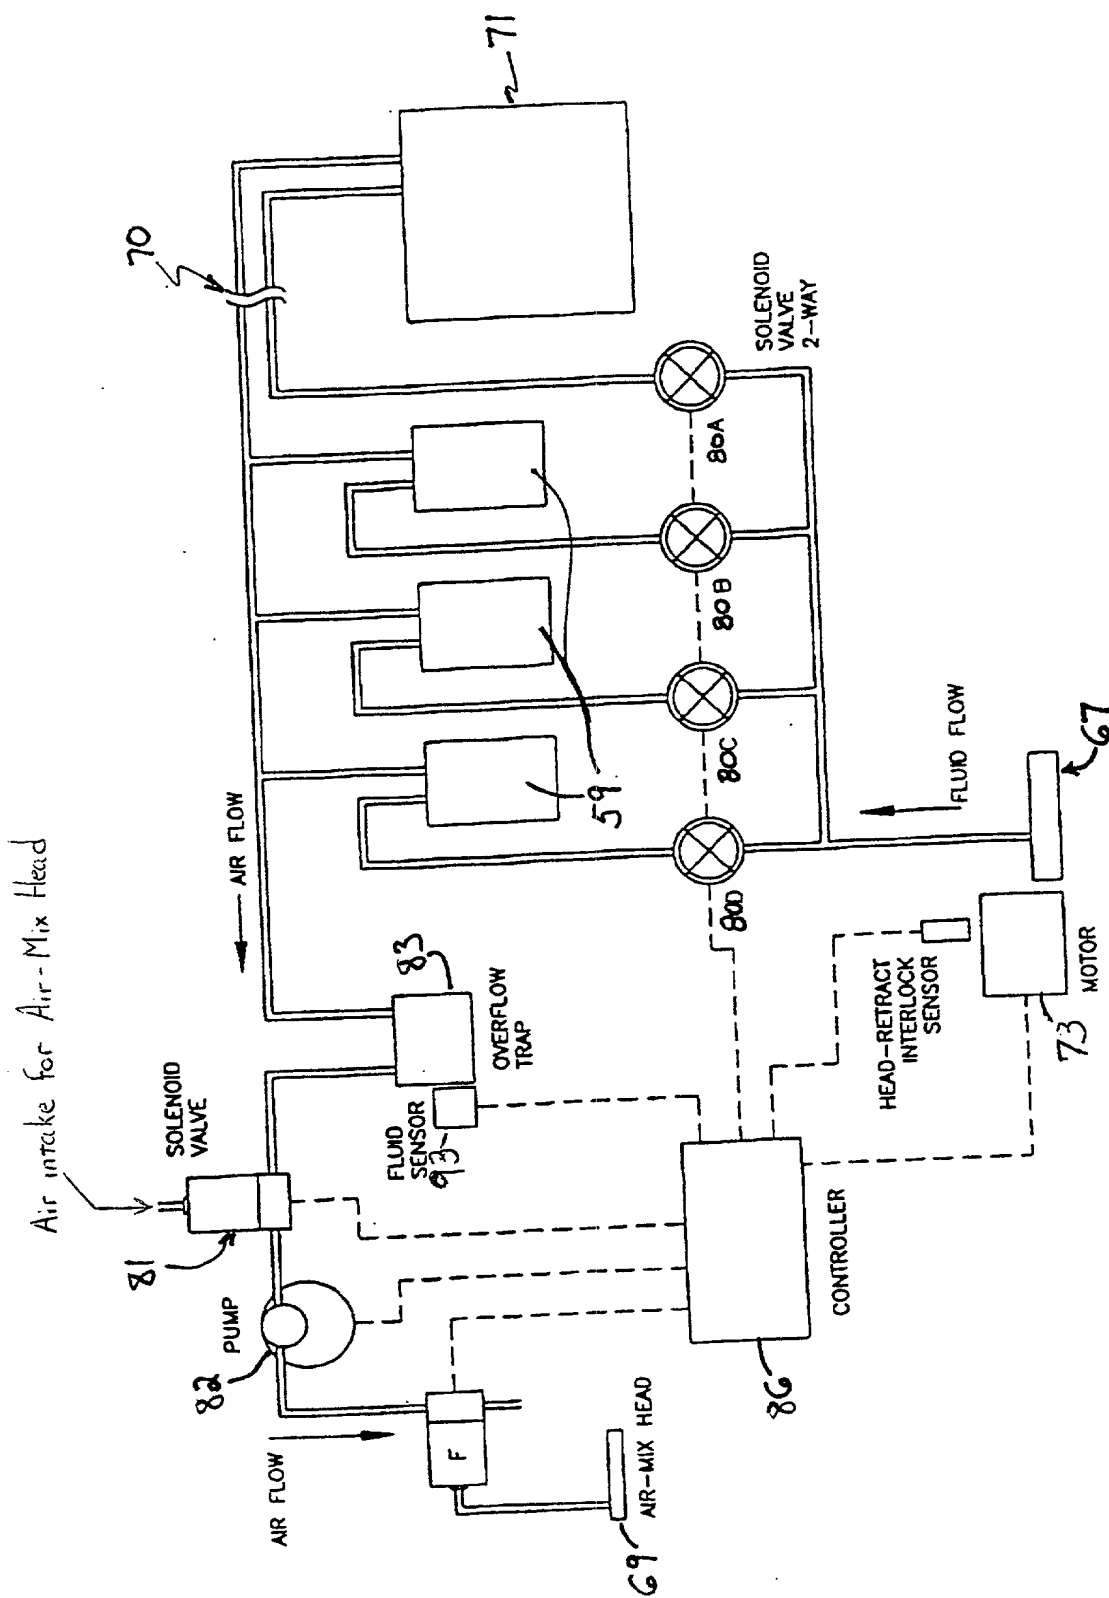


FIG. 15

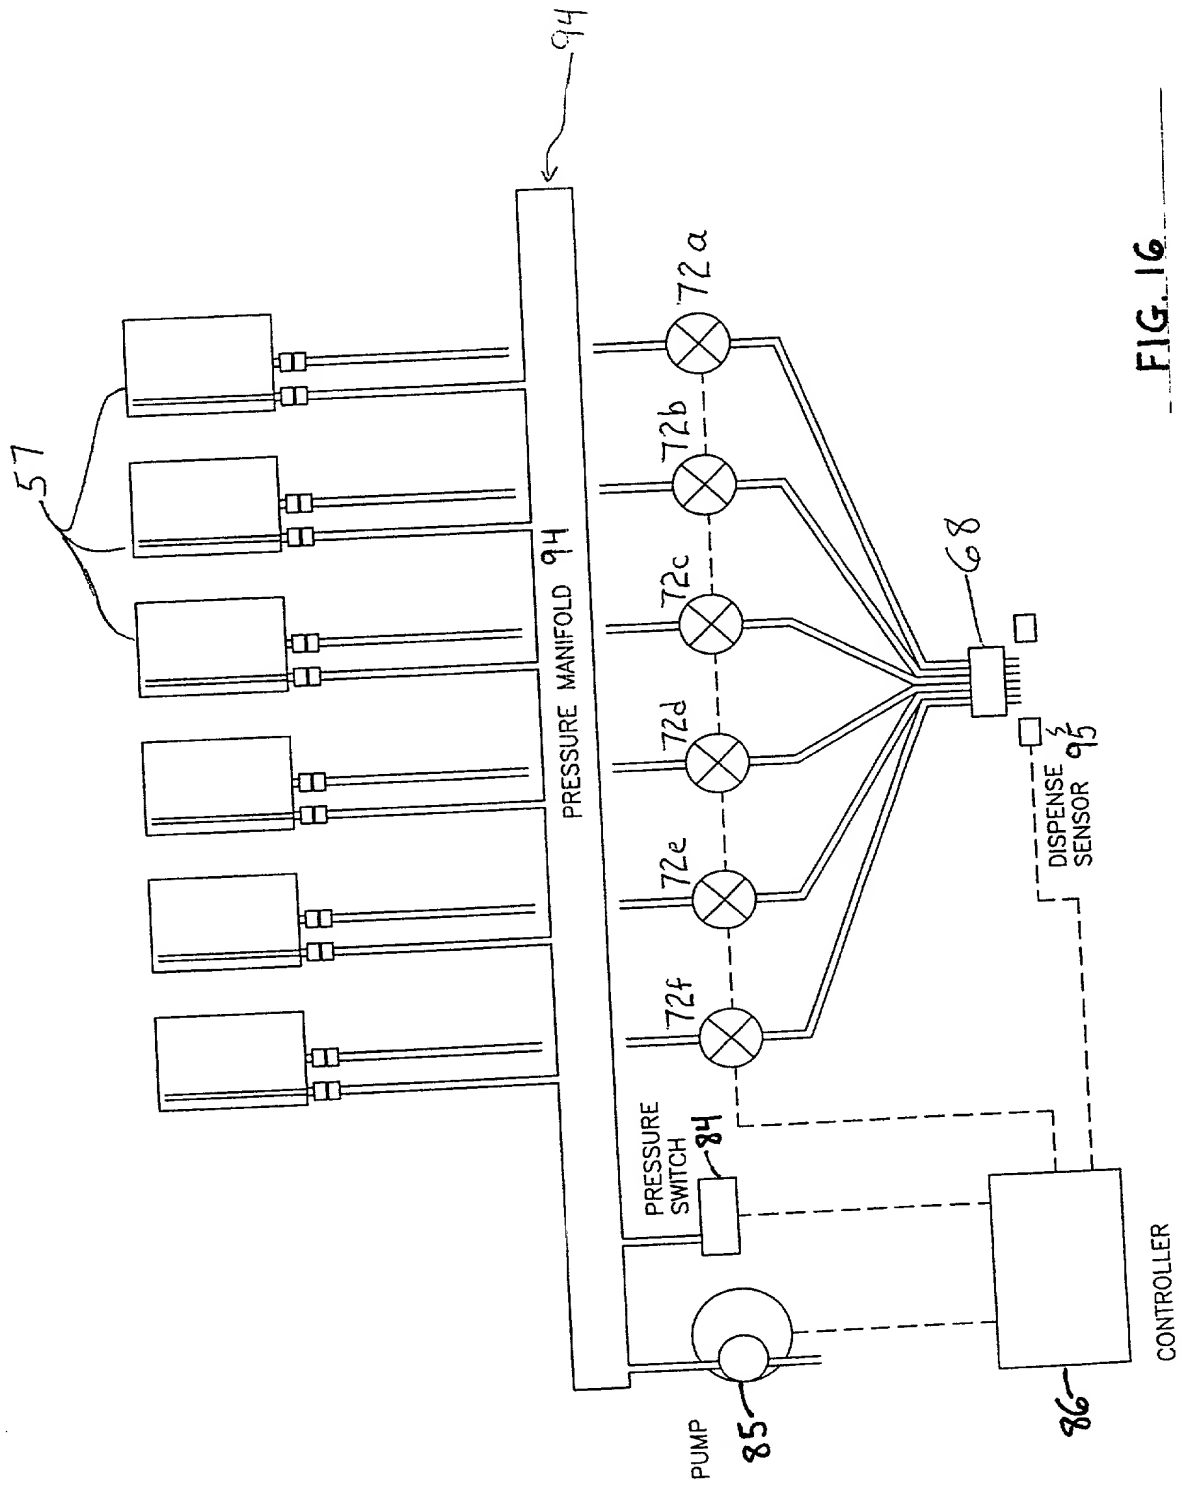


FIG. 16

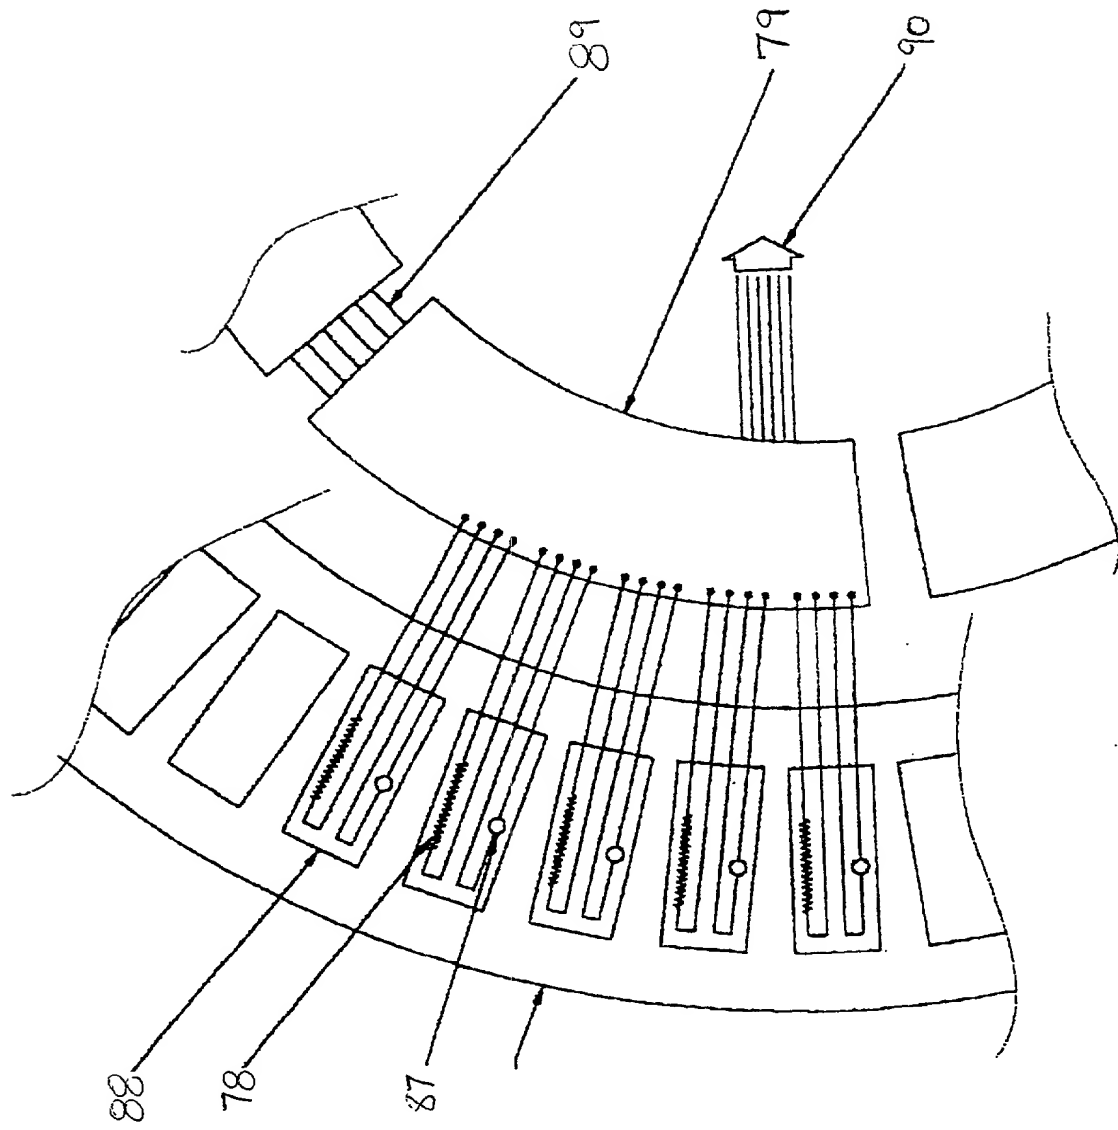


FIG. 17

862220-9292060

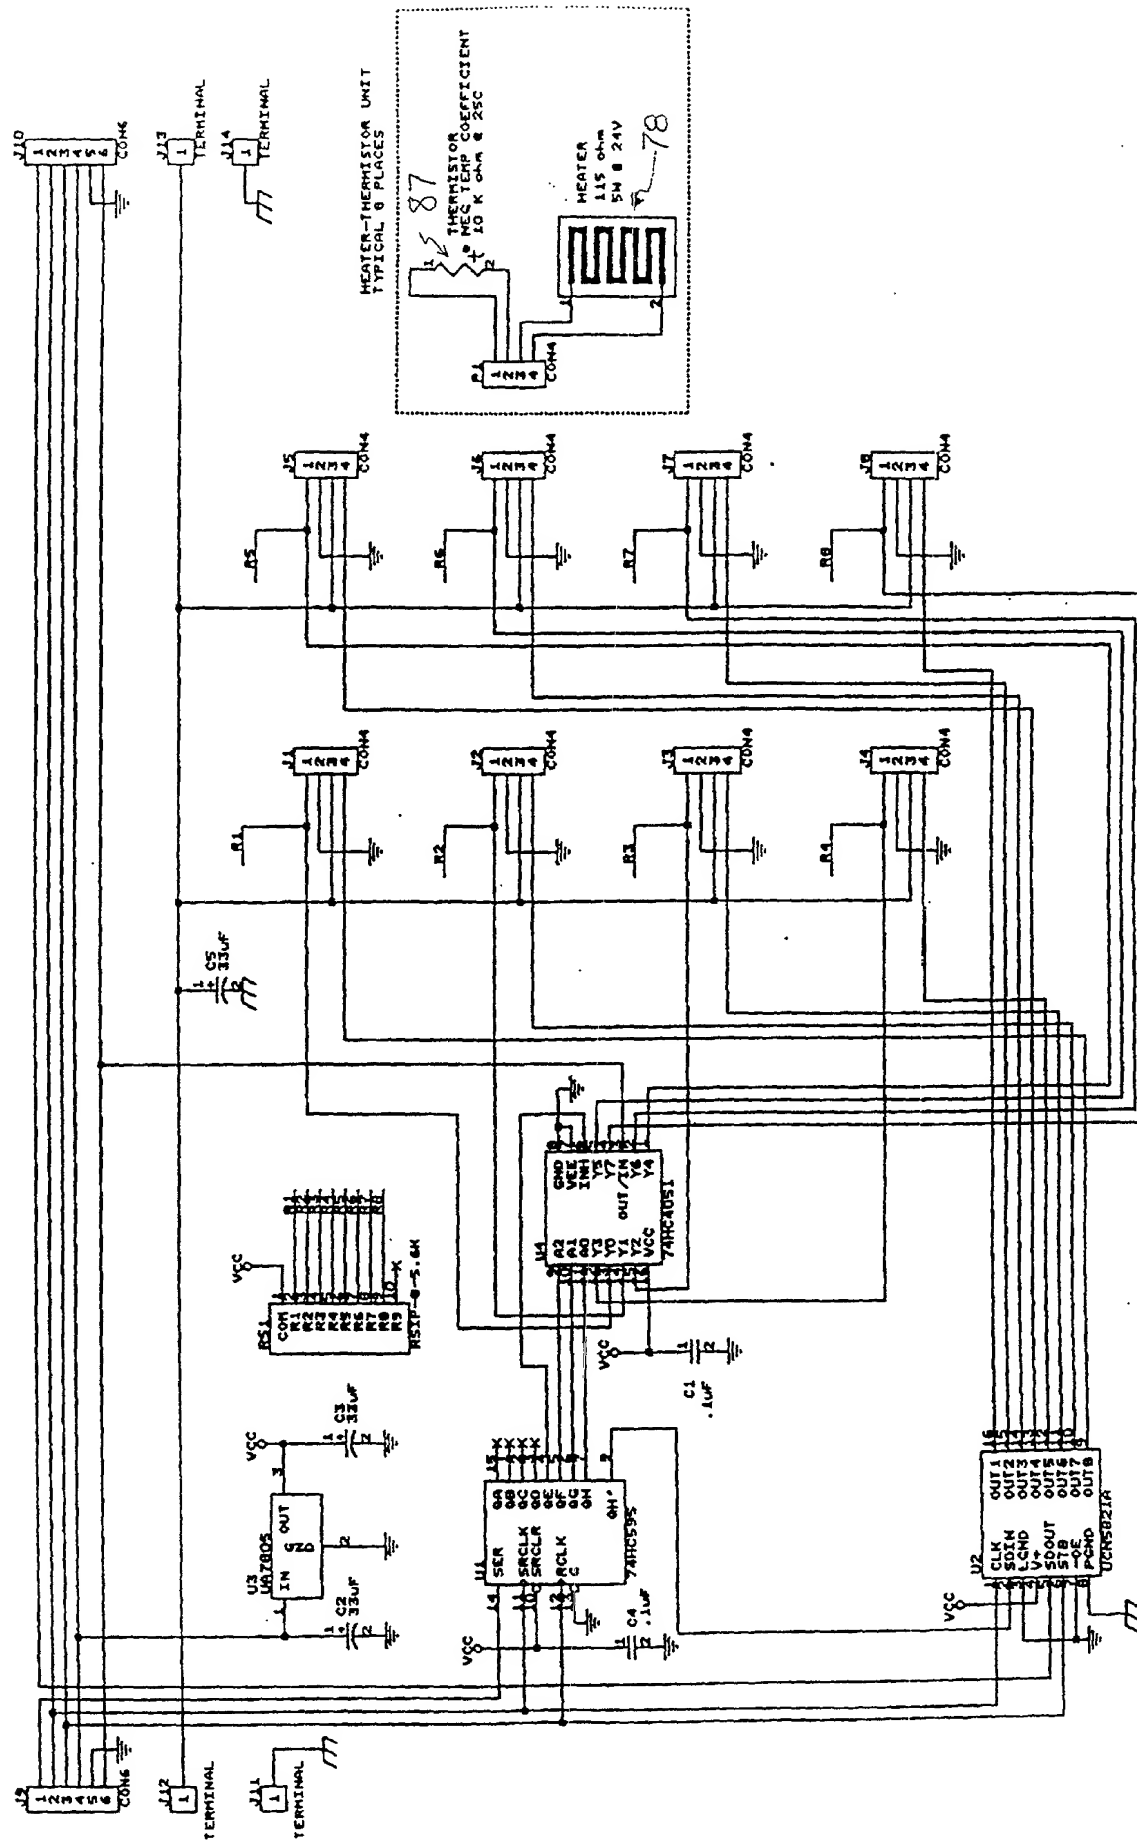


FIG. 18